
(12) UK Patent Application (19) GB (11) 2 031 142

- (21) Application No 7837906
- (22) Date of filing 23 Sep 1978
- (23) Claims filed 23 Sep 1978 19 Feb 1979
- (43) Application published 16 Apr 1980 (51) INT CL³ GO1F 1/70
- G01B 13/00
- (52) Domestic classification G1A A2 A3 C13 C4 D10 D2 EX G10 G1 G2 G7 R2 RX S10 S11 S6
- (56) Documents cited None
- (58) Field of search G1A
- (71) Applicant Robert F Shaw 135 Willowbrook Drive Portola Valley California 94025 **United States of** America


- (72) Inventor Robert F Shaw
- (74) Agents Eric Potter & Clarkson
- (54) Apparatus and method for examining a blood vessel of interest using radiation detected outside the body
- (57) Particulate sources of signals which can be detected outside the body of a patient are introduced into the circulating blood and are tracked in three dimensions in the region of the heart using suitable detectors (7, 7', 8, 8') disposed about the patient's chest. This permits the sequence of positions of each particle to be recorded as a function of time as each particle flows through a coronary vessel. Data analyses of these recordings of paticle positions provide information

about the velocity of blood flow through, and the course of each coronary artery. This velocity information is used to determine the extent, severity and location of stenotic lesions of the coronary arteries.

The sources preferably contain a positron emitter and their position is determined from produced pairs of

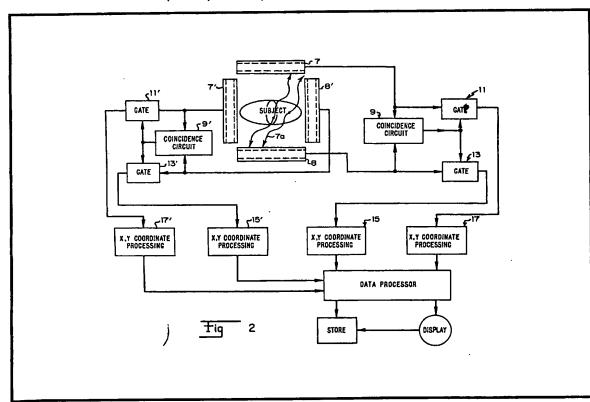


1/4

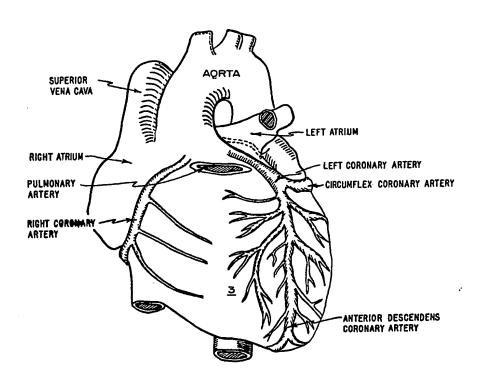



Tig

I

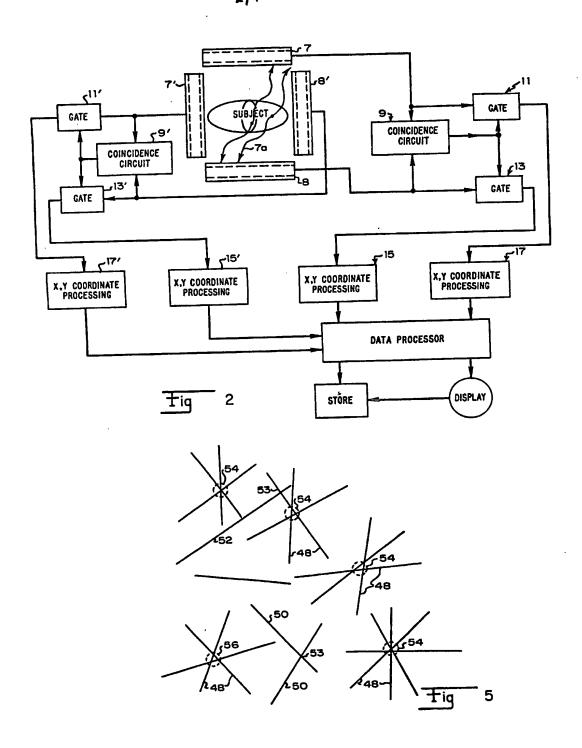

•

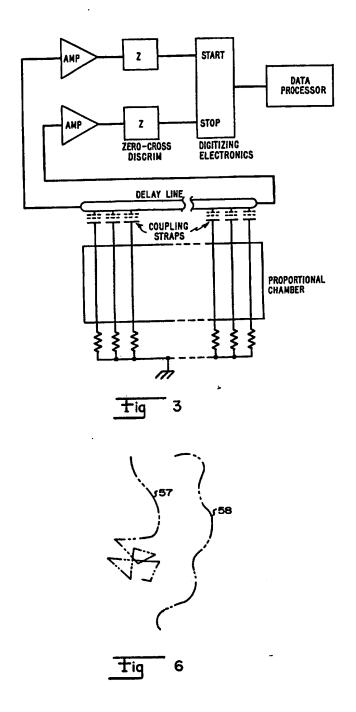

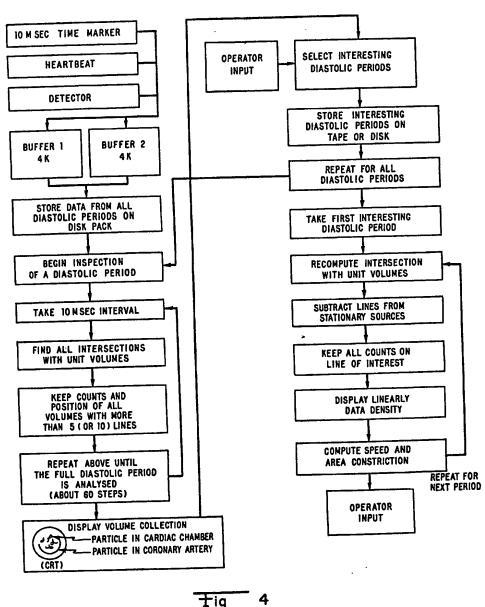

Tiq

SPECIFICATION

	Apparatus and method for examining a blood vessel of interest using radiation detected	
5	outside the body	5
3	This invention is concerned with apparatus and method for examining a blood vessel of interest using radiation detected outside the body.	
10	Coronary heart disease accounts for almost two-thirds of the deaths in the western world of adult males aged 30 to 64 years. Of all individuals sustaining their first myocardial infarction, more than half have had neither preceding signs nor symptons of coronary heart disease. It is therefore desirable to make early determinations of the existence, location and severity of coronary stenotic lesions in a manner that is convenient for the examination of a large number	10
15	of individuals. At present, coronary arteriography yields more useful information about the state of the coronary arteries than any other technique. However, the mortality rate and the incidence of major complications involved with this procedure are unacceptably high and the procedure is painful, expensive, and time-consuming. For these reasons, coronary angiography is not	15
20	performed upon asymptomatic individuals and is not suitable for screening large populations. In accordance with the present invention, stenotic artherosclerotic lesions of the coronary arteries are detected by injecting a number of particulate signal sources such as positron-emitting particles into the circulating blood of a subject to dtermine the velocity of blood flow through his coronary vessels.	20
25	Because of the high peripheral resistance of the myocardial vascular bed and the considerable range of auto-regulatory resistance changes available to the coronary circulation, coronary stenoses of 80%–90% are required to diminish the volume of coronary blood flow. This propensity of volumetric coronary blood flow to remain normal even in the presence of severe stenoses is responsible for the later occurrence or absence of anginal symptoms and diagnostic	25
30	electrocardiogram patterns, even in the presence of coronary stenoses, and explains why measurement of volumetric blood flow furnishes poor sensitivity in detecting coronary disease. However, this propensity of volumetric blood flow to remain normal even in the presence of severe stenosis furnishes a distinctive characteristic that blood flowing through a stenotic arterial	30
35	segment must have high velocity. In fact, to maintain the constant volumetric flow rate, the average fluid velocity within a stenotic segment of artery must change in strict inverse proportionality to the change in cross-sectional areas from normal to stenotic blood vessel. As coronary stenosis becomes more severe, the increments in blood flow velocity become progressively greater.	35
40	Discrete particulate signal sources such as positronemitting radioactive particles of sufficiently small size to pass through capillary beds are injected intravenously and become randomly distributed in the circulating blood volume. The particles are tracked in the three dimensions whenever they appear in the region of the heart by means of high resolution high-speed gamma detectors that surround the chest. These recordings of particle position as a function of time are analyzed and whenever a particle follows a flow path indicating that it is passing through a	40
45	coronary artery, the velocity of blood as it flows through the artery is measured by timing the transit of the particle. From the accumulated data of multiple particle transits through the coronary circulation, a three-dimensional representation of the lumen of the corronary arterial system is constructed.	45
50	In the accompanying drawings:— Figure 1 is a pictorial view of a human heart showing the principal coronary arteries: Figure 2 is a schematic diagram of the apparatus of the present invention showing the radiation detectors disposed about the region of the heart of a subject; Figure 3 is a schematic diagram of a conventional multi-wire proportional chamber which may be used as the detectors in the apparatus of Fig. 2;	50
55	Figure 4 is a process diagram showing operation of the data processor of Fig. 2; Figure 5 is a pictorial representation of data accumulated during a single time bin of operation according to the present invention; and Figure 6 is a pictorial representation of displayed data patterns representative of various	55
60	particle trajectories in and about the heart of a subject. There are three main coronary arteries which branch somewhat irregularly to form an average of ten secondary vessels, as shown in Fig. 1. Arteriosclerotic lesions are limited to the epicardial segments of the coronary vessels and rarely extend beyond the most proximal portions of the secondary vessels. The highest concentration of arteriosclerotic lesions is within the first 2 to 3 cm. of the left anterior descendens artery 3, but the lesions are otherwise rather randomly	60
65	distributed in the proximal primary and secondary arteries. Seventy percent of all arteriosclerotic coronary lesions are found within the proximal 4 cm. of the main coronary arteries.	65

5

20

25

30

35

40

45

50

65

order of 30 cm/sec. A 50% stenosis is generally considered to be significant. To be useful, the system should be capable of discriminating between normal vessels and 50% stenotic lesions and should be capable of assessing additional significant decrements of the cross sections of these vessels.

5 Typical blood flow velocities through stenoses of varying degrees are as follows:

	Degree of Stenosis	Average Velocity
10	0%	30 cm/sec
	50%	60 cm/sec
	60%	75 cm/sec
	70%	100 cm/sec
	80%	150 cm/sec
15	90%	300 cm/sec

Since nominal resting coronary flow velocity is about 30 cm/sec, ideally the system should be able to differentiate a flow velocity of 60–75 cm/sec for 30 cm/sec in order to detect 20 significant lesions and discriminate between velocities of 75, 100, 150, and 300 cm/sec in order to follow additional 10% increments in stenoses.

Positron-emitting particles are known which can travel some millimeters in blood or tissue before coming to rest. They will then be captured by an electron in the local tissue and both particles will be annihilated producing two gamma rays, each of 511 KeV moving in almost exactly opposite directions. The gamma rays can be detected at some distance with good spatial resolution, and a straight line joining the points at which the gamma rays were detected passes through their mutual point of origin and within a few millimeters of the positron-emitting source. By detecting a number of gamma pairs from a single stationary source, lines drawn between detected pairs will intersect at one point in space and define the position of the position-emitting source.

Typically, conventional detectors have spatial resolutions of the order of a centimeter. Since the organ being examined is normally stationary, additional resolution is obtained by observing a statistically large number of counts.

In accordance with the preferred embodiment, the present invention tracks a number of discrete moving positron-emitting sources present in the circulating blood. The system not only locates the position of the sources in three dimensions, but also locates them again and again at very short time intervals. The requirement as to how often a particle source must be located is determined from the following considerations.

As noted above, 30 cm/sec is about the nominal velocity of blood flow through a coronary 40 artery for a subject at rest. Blood flow through a diseased arterial segment which is 80% stenotic will have a velocity five times this nominal value (150 cm/sec). Blood flowing through a segment of a blood vessel with a severe 90% stenosis will have a velocity of the order of 300 cm/sec. In order to measure a 90% stenosis that is 1cm long, a particle moving through the stenosis should be detected at least a few times. At 300 cm/sec, only three milliseconds are 45 required to pass through a 1 cm length of vessel. If three determinations of position are desirable during this interval, a half-dozen coincident pairs of gamma rays must be detected during the three milliseconds and a minimum detection rate of 2,000 gamma pairs per second is indicated.

The detector of the present invention subtends about two-thirds of the total solid angle surrounding the heart. Each gamma ray has a 50% probability of leaving the body undeflected. There is thus a $(.5)^2 = .25$ probability that both members of a gamma pair will emerge from the body undeflected.

If the detecting element has a 20% efficiency for detecting a gamma ray incident upon it, then there is a (.20)² = .04 probability of detecting both members of a coincident pair.

55 Multiplying these numbers together furnishes the over-all probability that a positron annihilation 55 will produce a detected pair of

 $P = .67 \times .25 \times .04 = .0067$

60 Thus, it takes 150 annihilations on the average to produce one detected pair. For 2,000 60 detected gamma pairs per second, each source must emit 2,000 × 10 = 3 × 10⁵ positrons per second. 3.7 × 10⁵ positrons per second correspond to a 10 microcurie source, so individual source intensities on the order of 10 microcuries are indicated.

Sources of this or many times greater intensity are routinely available, but the particles used 65 in this application must be sufficiently small to pass through capillary beds, if they are to be

		injected by simple venipunctures and find their way to the coronary arteries. Fortunately, there exist a considerable number of positron emitters (such as Gallium ₈₈) which have half-lives of sufficiently short duration so that a small number of atoms produce a high decay rate. For example, Gallium ₈₈ has a half-life of only 68 minutes and can be readily, conveniently, and	
	5	inexpensively "milked" from Germanium ₈₈ , an isotope with about 270 days half-life. A pure Gallium source of one cubic micron volume has an intensity of 230 microcuries. While pure Gallium ₈₈ is unsuitable because it is a liquid at body temperature, the large carrier-to-active material ratios for particles having a short dimension less than 6-8 microns suggest that	5
	10	Gallium ₆₈ either compounded or absorbed in carrier particles would provide a suitable source. As noted above, there are three main coronary arteries which branch into an average of ten secondary branches. If, for statistical purposes, it is desired that three velocity measurements be made through each of the ten secondary branches, then a total $3 \times 10 = 30$ particle transists through the coronary system would be required. This would furnish approximately 10 transits through each of the proximal principal coronary arteries where most of the atheromatous lesions	10
	15	are located. Since coronary blood flow approximates only 5% of the cardiac output at rest, a given particle has only .05 probability of entering the coronary circulation after a single pass through the heart. Thus, 20 circulations through the heart times 30 particle transits through the coronary system, or a total of 600 particle transits through the circulation would furnish the redundancy	15
	20	of coronary blood flow velocity measurements outlined above. Since the mean circulation time is one minute or less, a single particle tracked in the circulation for 600 minutes would be suitable for the outlined redundancy, if its half-life were sufficiently long and if it continued to circulate for the ten-hour period. Of course, ten hours is an inconveniently long duration for a diagnostic measurement. Forty particles circulating for	20
	25	transit through the circulatory system. The number of particles required to attain 600 particle transits through the circulation is influenced by the possibility that the positron-emitting particles may be removed from the	25
	30	circulation by the Kupfer cells of the liver. The propensity of the liver to extract particles is a function of their size and surface characteristics, of the state of the reticulo-endothelial system as influenced by pre-treatment and otherwise, and a function of other variables. Liver blood flow is on the order of 20%-25% of cardiac output at rest. If particles are extracted by the liver with 100% efficiency, a total of 160 particles would have to be	30
	35	administered and the examination conducted for a fifteen-minute period in order to furnish the desired 600 circulatory transits under these circumstances. A reasonable program of particle administration might begin with an initial intravenous injection of 50 particles, with 12 particles injected at the end of each of nine subsequent 1-minute periods. Alternatively, if particles are extracted from the liver with less than 100% efficiency, the number of particles required for a	35
	40	exposure of the patient and the complexity of the data processing required. If liver extraction is 100% efficient, the total administered dose is 160 particles × 10 microcuries per particle = 1.6 milliouries, which compares favorably with the 2 milliouries Gallium, dose currently administered	40
	45	for bone scanning. Radiation to the liver for this worst case is 3 rads, which compares favorably with the liver dose of 6 rads which results from conventional liver scans using Gold ₁₉₈ . However, if the circulating particles are not picked up by the liver during the fifteen-minute examination time, only 40 particles constituting 0.4 millicurie need be administered. Since Gallium ₆₈ has a radioactive half-life of only 68 minutes, if the circulating particles are not extracted by the liver	45
•	50	over a period of a few hours, radiation of the liver is essentially zero and radiation to the rest of the body is so widely dispersed as to be negligible. The complexity of data processing is significantly influenced by the number of particles that must be simultaneously detected in the field of view which encompasses the heart. The coincidence circuit 9 and gates 11, 13, shown in Fig. 2, connected to the gamma detectors 7, 8 of the type shown in Fig. 3, constitute a preprocessing circuit that accepts only those gamma	50
		rays which occur as synchronous pairs and which emerge from the general region of the heart. The field of view of detectors 7 and 8 thus situated contains only 5%-7% of the total blood volume. Even if the efficiency of hepatic extraction is 100%, the total number of particles in the entire circulating blood volume at any one time need be no more than 50 to obtain the highly and the state of massuraments described above. Under these extreme circumstances, no	55
	60	more than 3-4 particles need be in the field of view at any one time, a very acceptable number for uncomplicated data processing. The detectors 7 and 8 consist of two or more pairs of detecting modules, for example, of the thorax as shown in Fig. 2, and locate the arriving	60
	65	gamma rays to an accuracy of about a millimeter. This information, which exists in the form of electrical pulses, is stored, say on tape or disc, depending on the rate of events, for	65

subsequent computer processing. As noted, only gamma rays that arrive synchronously on opposing detectors 7 and 8 in Fig. 2 and only synchronous pairs that could have originated in the region of the heart are accepted for recoring. Thus, gamma rays 7a that arrive synchronously from a region beyond the heart may be conveniently rejected as irrelevant data. 5 Subsequent computer processing of the stored data constructs straight lines in space corresponding to the inferred flight paths of the recorded gamma rays as represented in the pictorial presentation of Fig. 5. Three times out of four, at least one of the gamma rays will have been Compton scattered, producing a line 50 which does not pass through the point at which the gamma rays actually originated. These lines 50 are rejected in the data analysis because 10 10 they do not consistently intersect other lines in the region of the same slowly-moving point in space. Intersections of the "true" lines will cluster together near one point 54 in space, corresponding to location of a source at a given time, which moves with a velocity of a few tens or hundreds of cm/sec. The intersections 53 of "spurious" lines are scattered randomly about and do not converge near any point. It is desirable to minimize this background clutter of spurious lines against which the sources 15 must be "seen", since the "true" lines do not pass through a perfect point of intersection, but through a region of ambiguity of a few millimeters in size, smeared by the variable distances and directions in which the positrons move from the source before annihilating and by the motion of the surface of the heart, where the coronary arteries of interest are located. In 20 20 accordance with the present invention, the system can be operated through synchronized gates in order to observe sources only during the diastolic phase of the cardiac cycle when heart motion is least and the velocity of blood in the coronary arteries is greatest and most constant. Cardiac diastole characteristically occupies 400-600 milliseconds, which is considerably longer than the transit time (30-300 milliseconds) required for a particle to flow through a 10 cm 25 length of coronary artery. As a result, data may be accumulated during a single diastolic period 25 to provide a plurality of ray-intersection "clusters", as representing pictorially in Fig. 5. Further computer processing of the intersections of the "true" straight lines reconstructs the positions of the positron-emitting sources in three dimensions as a function of time as they passed in the circulating blood through the field of view of the pairs of detector modules 7, 8 of 30 Fig. 2. These intersections are accumulated in a number of time bins and are reconstructed to 30 represent to flow paths of the particles. In practice, an operator may conveniently interface with the computer during this phase of data analysis to discriminate between the flow paths which represent transit through a coronary vessel and the flow paths which represent entrance to and exit from the chambers of the heart. This type of operator discrimination is simplified by the fact 35 35 that these two kinds of flow paths are quite different, both spatially and with respect to relative flow velocities during the various phases of the cardiac cycle, and by the fact that an average of only three to four particles are typically in view at any one time. In operation, then, an event is accepted by the hard-wired electronics if a signal is received at two detector chambers within about 50 nanoseconds and if the spatial locations of the two 40 chambers indicate the event originated in a small volume encompassing the heart. These events 40 may be stored, for example, in a disc memory device. The information thus stored may typically consists of 20 bits for the x, y coordinates for each side of the detector, and 4 bits for gap identification within the module, if a multiple layer multiwire proportional chamber is used as the detector. Thus, each event (a synchronous pair of 45 gamma rays) may require four 12-bit words to identify it. In addition, ECG information and a 10 45 millisecond time marker may be stored on the disc to allow for correlation between the event and the cardiac cycle. Analysis may then be performed by the following steps: Starting with the onset of cardiac diastole, the data can be divided into 10 millisecond time bins. Each bin may be analyzed on a 10 by 10 by 10 cm3 matrix where the unit volume is 1 50 cubic cm. Each intersection of two or more lines (corresponding to the synchronous pair of 50 gamma rays) within a unit volume is stored as an event and only those unit volumes with more than 5 (or 10) events stored in them will be selected. On the average, not more than two to five unit volumes will satisfy this criteria for each time bin. Storage may be provided for ten of them. The counts in the unit volume selected and its position may thus be stored separately and the 55 process will be repeated for the next 10 millisecond period. Once all intervals within a diastolic 55 period are analyzed, the inter-sections representative of the positions of the particles can be displayed sequentially, as shown pictorially in Fig. 6, for all time bins during a diastolic period. Particles that were resident in the cardiac chambers during diastole exhibit characteristic lines 57 having short random segments. Particles that flowed through a coronary vessel during 60 diastole exhibit a long line 58 of characteristic contour corresponding to the course of a 60 coronary artery. An operator may view these data patterns which represent transits of particles in and about the heart and perform simple data selection based upon the geometry of the flow transit paths 57, 58. Data corresponding to particles which passed through a coronary artery are selected and data corresponding to particles which entered into and resided in a cardiac 65 chamber (or took some other extra-coronary path such as through a lung) are rejected. 65

5	on an effectively expanded particle with greater time events per unit volume we particle with respect to titotal course of the flow particle with the flow parti	for each path of interest during a diastolic period can be redisplayed and time scale in order to determine the sequential location of each resolution. In stenotic regions of faster blood flow, a lower number of will be encountered and this information about sequential locations of a me is used to determine the relative velocities of a particle over the eath along the coronary artery. Peated for all diastolic periods of the examination and, from the lated, the existence, location, severity and extent of stenotic and dilated	5
10	regions of the coronary arteries can be determined. One important constraint governing the suitability of a positron source concerns the energy of the positrons emitter. It is desirable to limit the range that the positron travels in tissue before application and conversion to gamma pairs in order to minimize the sphere of confusion in		
15	inferring the radionuclide position from intersection of the lines-of-flight of gamma pairs. Since the range of 1 MeV positron is about 0.5 gm/cm² or 5mm in tissue, it is desirable to have the mean positron energy below 1 MeV. The circulating particles should be no larger in their 1 smallest diameter than 6–8 microns so that they will freely pass through capillary beds and each particle should produce at least 3 × 10 ⁵ positrons per second. The specific activity (number		
20	of radioactive decays/second/gram) of a radionuclide required to turnish this positron rate in a particle of the small size indicated will depend upon the physiochemical properties of the radionuclide and the manner in which it forms particulates with carrier materials. The specific activity of a radionuclide is inversely proportional to its half-life. Acceptable half-lives must take into account the method of production of the radionuclide and the time required to chemically or obvisionly convert the radionuclide into suitable particle form.		
25	Gallium _{es} is an attracti	ve source candidate, because of its following radioactive properties:	25
	half-life decay product	68 minutes stable ⁶⁸ Zn	
	modes of decay	88%+ of which 86% goes	
30	mean positron energy	to ground state of ⁸⁸ Zn 1 MeV	30
	production	from decay of Germanium _{es} , which has a half-life of 275 days	
35	Gallium ₆₈ is a short-lived daughter continually produced by a long-lived parent. Germanium ₆₈ "cows" are commercially available at low cost (less than \$1,000 for the specific activity required for the worst case discussed above). The Gallium ₆₈ produced by these generators is conveniently removed from the Germanium cow by eluting with an aqueous EDTA solution. Ga ₆₈ can be liberated from the GaEDTA complex by mixing with a strongly acetic iron solution or		
40	Gallium is a chemicall	y highly reactive element which readily forms many inorganic, insoluble	40
45	complex is (Ga) (Cr)(PO ₄ Ga ₆₈ -EDTA complex and conventionally pulverize administration. Of cours present invention. For ex- the detection may be pe) ₂ , formed by adding a phosphate buffered chromic salt to the eluted boiling away the EDTA and water. The resulting crystals may be d and screened to the requisite size in a diluent suitable for intravascular e, other radiation-emitting sources may be used in accordance with the xample, particular X-ray sources may be introduced into the blood and erformed by recurring exposures for brief intervals of photographic film	45
50	The detector system of	prax of a patent. consists of one or more pairs of modules 7, 8, 7', 8', preferably arranged (consists as shown in Fig. 2, Each module 7, 7', 8, 8' may be a	50
55	sandwich of five multi-we conventional design. Su of 5 cm. The .511 MeV annihilation vectors are 2). Design of synthesis are of this typ	vire proportional chambers coupled to 1 mm lead converters according to 1 ch modules have an active area of 50 cm × 50 cm and a total thickness of annihilation photons are converted to electronis in the lead and the determined from two opposing multi-wire proportional chambers (Fig. e, where multiplication without sparking is used to determine the less ribed in the literature (see, for example, Charpak, et al., Nucl. Inst.	55
60	Methods 62:262, 1968; 65:217, 1968; 88:149, 1970). Detectors of this type may consist of three-wire grids with the central grid held at a positive d.c. voltage with respect to the outer two grids. For the purpose of gamma ray imaging, one of the outer grids is replaced by a lead converter which is placed very close to the high voltage grid (≈1 mm). The two grids have wires at right angles to each other and can be placed further apart (5–10mm). The conversion electrons in passing through the gas in the chamber produce electron-ion pairs. These electrons		
65	are condensted towards	a positive high voltage wire, undergoing rapid multiplication in the high the wire. This results in a voltage pulse on the wire. A similar pulse is	65

65 the cardiac cycle of the subject.

65

induced on the wires of the ground plane. Determining the wires on which these pulses occur gives the spatial location of the event. This may be done by capacitively coupling the wire grids to delay lines, as shown in Fig. 3. Measuring the time difference between the generation of the pulse and its arrival at the end of the delay line indicates the position of the origin of the pulse on the delay line and thus the spatial location of the event. The present technique allows spatial location accuracy of 1mm, data rates of over 105/second and resolving times of the order of 30-60 nano-seconds. Of course, the wire grids may all be coupled to a central processing unit or computer for direct determination and location of simultaneously occurring pairs of annihilation photons. Even for pure positron-emitting sources, the majority of detected events consists of a single 10 gamma ray, the other escaping the system because of its limited acceptance and detection efficiency. Also, some of the annihilation photons may convert in tissues surrounding the source, thus further reducing potential coincidence counts in both detectors. Considering only the hardware-related part of this problem and including a factor of .25 for 15 Compton scatter of the annihilation photons, for identical detectors 7 and 8 mounted 15 symmetrically on four sides of a cube, as shown in Fig. 2, we may define: G as the geometric acceptance of the system for the particular source position e as the efficiency for the detection of a single 511 KeV photon N as the number of annihilations per second occurring at the source 20 20 au as the resolving time of the chamber For the case of a pure positron emitter, we set: G = .66e = .20 $\tau = 50 \times 10^{-9} \text{ sec}$ 25 N = 10 microcurie $Ci = 3.7 \times 10^5$ sec The rate of accidentical coincidences A due to the detection of two uncorrelated events is: $A = G^2 e^2 N^2 \tau = 125/sec$ which is distributed almost uniformly over the field, causing a low background data density. The number of real events R is: $R = .25Ge^2N = 2.5 \times 10^3/sec$ 30 concentrated over a small volume. The singles average data rate at each chamber is: $\frac{G}{2} \times \frac{e}{5} \times N = 4.8 \times 10^3 / \text{sec}$ 35 which is well within the capabilities of such a detector. CLAIMS (23 Sep 1978) 40 1. Apparatus for interacting with a number of particles which can be introduced into the blood of a subject and which can provide signals from within a vessel of interest that can be detected outside the body, the apparatus comprising: detector means positionable near the body of the subject for detecting the signals from the number of particles at successive locations of each of the number of particles at successive 45 45 times during the travel of each particle through a vessel of interest; circuit means coupled to said detector means for providing output manifestations from successive positions of each of the number of particles at successive times during the travel thereof through the vessel of interest; and output means responsive to the output manifestations from said circuit means for providing an 50 50 indication of the relative internal cross-sectional areas of the vessel of interest at sucessive positions along the course of the vessl of interest. 2. Apparatus according to claim 1 for interaction with a number of particles which can produce radiation that passes through the body walls of the subject; and wherein: said detector means is positionable near the body of the subject for receiving the radiation 55 emanating from the body of the subject to produce electrical signals in response thereto. 55 3. Apparatus as in claim 2 wherein said circuit means includes input means connected to receive electrocardiographic signals from the subject for controlling said circuit means to selectively respond to said electrical signals from the detector means during a selected portion of the cardiac cycle of the subject. 4. Apparatus as in claim 3 wherin said circuit means includes coincidence means and timing 60 means connected to control said circuit means for producing data signals representative of the occurrence and locations of pairs of electrical signals produced by said detector means during each of a plurality of time intervals determined by said timing means and occurring as determined by said coincidence means in substantial coincidence within said diastolic portion of

	5	5. Apparatus as in clam 2 wherein said circuit means includes gate means and coincidence means connected thereto for controlling the transmission therethrough of only electrical signals from said detector means which are indicative of substantially oppositely propagating gamma rays that are received from the body of the subject within a selected time interval of separation between occurrences.	5
		6. Apparatus as in claim 5 wherein said coindence means controls said gate means to transmit therethrough only the electrical signals produced by said detector means within a time interval of not greater than 50 nanoseconds.	
•	10	7. Apparatus as in claim 5 wherein said circuit means includes gate means and coincidence means connected thereto for controlling the transmission therethrough of only coincident electrical signals produced by said detector means in response to oppositely-directed pairs of gamma rays received thereby along a straight line which may intersect a vessel of interest in the body of a subject about which the detector means is positioned.	10
•	15	O Apporatus as in claim 2 wherein said detector means produces electrical signals in	15
	20	millimeters. 10. Apparatus as in claim 1 wherein said circuit means includes timer means for providing said output manifestations from each of said particles in the vessel of interest at successive times occurring at approximately one to ten millisecond intervals.	20
		11. Apparatus as in claim 1 wherein said detector means is capable of being positioned to within approximately two-thirds solid angle around the heart of said subject. 12. Apparatus according to claim 1 for interaction with a number of particles which produce gamma rays that pass through the body walls of the subject, and wherein	
	25	said detector means is positionable near the body of the subject for receiving gamma rays emanating from the body of the subject to produce electrical signals in response thereto. 13. Apparetus according to claim 12 wherein said detector means includes portions which	25
	30	are positionable near the body of the subject for receiving gamma rays emanating in substantially opposite directions from the subject to produce electrical signals in response thereto. 14. Apparatus as in claim 1 wherein said circuit means includes data storage means for	30
	35	recording said output manifestations of each of the number of particles as a function of time. 15. Apparatus for interacting with a number of particles which can be introduced into the blood of a subject and which can provide signals from within a vessel of interest that can be detected outside the body, the apparatus comprising:	35
	30	detector means positionable near the body of the subject for receiving the signals emanating from the body of the subject to produce electrical signals in response thereto which are indicative of the successive locations of a particle from which the received signals emanated	
	40	from the body; circuit means responsive to said electrical signals for providing output manifestations indicative of the three-dimensional coordinates of successive locations of each of said particles within said vessel of inerest as a function of time; and output means responsive to the output manifestations from said circuit means for providing an	40
	45	indication of the course of the vessel. 16. Apparatus according to claim 15 for interaction with a number of particles which can	45
•		emanating from the body of the subject to produce electrical signals in response thereto.	50
j	50	are positionable near the body of the subject for receiving gamma rays emanating in substantially opposite directions from the subject to produce electrical signals in response thereto. 18. Apparatus according to claim 15 for interaction with a number of particles which can	
	55	produce radiation that passes through the body walls of the subject; and wherein:	55
	60	coincidence means connected thereto for controlling the transmission therethrough of only electrical signals from said detector means which are indicative of substantially oppositely propagating gamma rays that are received from the body of the subject within a selected time	60
		interval of separation between occurrences. 20. Apparatus as in claim 18 wherein said detector means produces electrical signals in response to gamma rays received thereby of approximately .5 MeV. 21. Apparatus as in claim 18 wherein said detector means has a resolution of at least about	
	65	21. Apparatus as in claim 18 wherein said detector means has a resolution of at least about 5 millimeters.	65

	22. As a set of the claim 10 subardia and as a side of the control and make make the	
	22. Apparatus as in claim 19 wherein said coincidence means controls said gate means to transmit therethrough only the electrical signals produced by said detector means within a time interval of not greater than 50 nanoseconds.	
	23. Apparatus as in claim 19 wherein said circuit means includes gate means and	
5	coincidence means connected thereto for controlling the transmission therethrough of only	5
	coincident electrical signals produced by said detector means in response to oppositely-directed	
	pairs of gamma rays received thereby along a straight line which may intersect a vessel of	
	interest in the body of a subject about which the detector means is positioned. 24. Apparatus as in claim 15 wherein said circuit means includes timer means for providing	
10	said output manifestations from each of said particles in the vessel of interest at successive	10
, 0	times occurring at approximately one to ten millisecond intervals.	
	25. Apparatus as in claim 15 wherein said detector means is positioned to within	
	approximately two-thirds solid angle around the body of the subject.	
	26. Apparatus as in claim 15 wherein said circuit means includes data storage means for	
15	recording said output manifestations of each of the number of particles as a function of time.	15
	27. Apparatus as in claim 15 wherein said circuit means includes input means connected to	
	receive electrocardiographic signals from the subject for controlling said circuit means to	
	selectively respond to said electrical signals from the detector means during a selected portion of the cardiac cycle of the subject.	
20	28. Apparatus as in claim 27 wherein said circuit means includes coincidence means and	20
20	timing means connected to control said circuit means for producing data signals representative	
	of the occurrence and locations of pairs of electrical signals produced by said detector means	
	during each of a plurality of time intervals determined by said timing means and occurring as	
	determined by said coincidence means in substantial coincidence within said diastolic portion of	
25	the cardiac cycle of the subject.	25
	29. Apparatus for interacting with a number of particles which can be introduced into the	
	blood of a subject and which can produce radiation from within a vessel of interest that passes through the body walls of the subject in substantially opposite directions from the location of the	
	particle within the body, the apparatus comprising:	
30	detector means positionable about the body of the subject for receiving the radiation	30
••	emanating in substantially opposite directions from the body of the subject to produce electrical	
	signals in response thereto which are indicative of successive locations of each of the number of	
	particles at successive times during travel of each particle through the vessel of interest; and	
	circuit means including timing means coupled to said detector means for providing output	25
35	manifestations indicative of the three-dimensional coordinates of successive positions of each of	35
	the number of particles which is within the vessel of interest and from which the detector means receives oppositely-directed radiation in substantial coincidence during a time interval deter-	
	mined by said timing means, said circuit means including signal selecting means connected to	
	receive said output manifestations for producing an output therefrom in response to the	
40	occurrence of at least three pairs of coordinates represented by said output manifestations for a	40
	selected time interval attaining values which correspond to at least three straight lines	
	connecting such pairs of coordinates substantially intersecting at a location within the vessel of	
	interest, thereby to identify the location of a positron-emitting particle in the vessel of interest,	
4 6	and output means responsive to the outputs from said signal selecting means for providing an indication of successive positions of a particle along the course of a vessel of interest.	45
45	30. Apparatus as in claim 29 wherein said circuit means includes display apparatus	73
	responsive to the outputs from said signal selecting means for providing an output indication of	
	sequential locations as a function of time of said intersections to provide an indication of the	
	relative internal cross-sectional areas of the vessel of interest at successive positions along the	
50	course of the vessel of interest.	50
	31. Apparatus as in claim 29 wherein said circuit means includes data processing means	
	responsive to the successive locations during each of said time intervals of said intersections representing a particle for indicating the relative cross-sectional areas at various locations along a	
	vessel of interest, thereby to determine the existence, severity and location of stenotic or dilated	
55	regions of said blood vessel.	55
•	32. Apparatus as in claim 29 wherein said circuit means includes display apparatus	
	responsive to the outputs from said signal selecting means for providing an output indication of	
	sequential locations as a function of time of said intersections to provide an indication of the	
	course of the vessel of interest.	00
60	33. Apparatus as in claim 29 wherein said circuit means includes data processing means	60
	responsive to the successive locations during each of said time intervals of said intersections representing a particle for indicating the course of the vessel of interest.	
	34. The method for determining the course of a blood vessel of interest within the body of a	
	subject, the method comprising the steps of:	
65	introducing into the blood stream of the subject one or more particles capable of providing	65

	signals detectable from outside the body to flow with the blood through the blood vessel of	
	interest; establishing a field of detection which encompasses the blood vessel of interest and tracking through the field of detection the successive locations of each particle as it flows through the	_
5	blood vessel of interest; and	5
	determining therefrom the course of the vessel of interest. 35. The method according to claim 34 wherein in the step of introducing, the particles are	
	introduced by peripheral venous injection to pass through the capillary beds of the body of the	
	subject to be detected in an artery of interest.	
10	36 The method according to claim 34 wherein in the step of introducing, particulate	10
	sources of radiation which can produce radiation that can pass through the body walls of the subject are introduced into the blood stream, and comprising the step of detecting radiation. 37 The method as in claim 36 wherein in the step of detecting, detecting only pairs of	
	gamma rays received from the body of the subject in substantial coincidence from substantially	15
15	opposite directions with respect to the selected vessel to produce said signals indicative of said	
	locations. 38. The method for determining the course of a blood vessel of interest within the body of a	
	subject the method comprising the steps of:	
	introducing into the blood of the subject a number of particulate sources of radiation which	20
20	can produce radiation from within a vessel of interest that can pass through the body walls of	20
	the subject; detecting the electrocardiographic signals from the subject to identify therefrom the diastolic	
	portion of the cardiac cycle of the subject:	
	detecting the radiation emanating from the body of the subject only during said diastolic	25
25	portion of the cardiac cycle to determine the three-dimensional source; and	25
	determining therefrom the course of the vessel of interest within the body of the subject. 39. The method for determining the course of a blood vessel of interest within the body of a	
	subject, the method comprising the steps of:	
	introducing into the blood of the subject a number of particulate sources of radiation which	20
30	can produce radiation from within a vessel of interest that can pass through the body walls of	30
	the subject; detecting only pairs of gamma rays received from the body of the subject in substantial	
	coincidence from substantially opposite directions with respect to the Vessel of Interest;	
	selecting pairs of substantially coincident, oppositely-directed gamma rays which have	35
35	goodinates for each pair that correspond to the substantial intersection of three straight lines	39
	connecting said coordinate pairs, each of these intersections occurring at a location within a vessel of interest to identify the successive locations of a positron-emitting particle flowing	
	thorewithin: and	
	determining therefrom the course of the vessel of interest within the body of the subject.	40
40	40. The method according to claim 39 including the step of accumulating the number of	40
	pairs of substantially coincident, oppositely-directed gamma rays whose coordinates are associated with said intersections occurring during successive time periods.	
	41. The method as in claim 40 including the step of displaying the successive locations of	
	the flowing positron-emitting particles to indicate therefrom the course of the vessel of interest.	4.5
45	42 The method for determining the existence, location and severity of stenosis or dilations	45
	of regions of selected blood vessels within the body of a subject, the method comprising the	
	steps of: introducing into the blood of the subject a number of particulate sources of radiation which	
	can produce radiation from within a vessel of interest that can pass through the body walls of	
50	the subject:	50
	detecting the radiation emanating from the body of the subject to determine the successive locations of the radiation source and the relative frequency of occurrence of the detected	
	radiation:	
	determining therefrom the course of the vessel of interest within the body of the subject and	
55	the relative frequency of occurrence of detected radiation per unit length along the course of the	55
	word of interest; and	
	ascertaining therefrom the relative internal cross-sectional areas of the vessel of interest from the direct relationship thereof to the frequency of occurrences of detected radiation per unit	
	length of the vessel of interest.	
60	A3 The method as in claim 42 wherein the step of introducing particulate sources,	60
	introducing particulate sources of positrons having energy levels not higher than approximately	
	1 MeV. 44. In the method according to claim 42, the additional steps of detecting the electrocardi-	
	paraphic signals from the subject to identify therefrom the diastolic portion of the cardiac cycle	
65	of the subject, and limiting the step of detecting the radiation emanating from the body of the	65

-	subject only during said diastolic portion of the cardiac cycle. 45. The method as in claim 44 wherein the output indication is produced in response to data manifestations representative of the occurrence and detection locations of gamma rays detected in substantial coincidence during selected time periods within the diastolic portion of	5
5	the cardiac cycle of the subject. 46. The method as in claim 44 wherein producing said output indication comprises the additional step of storing the data manifestations during each time period for producing an output indication for each time period during which the number of said occurrences exceeds a value greater than one.	
10		10
15		15
20	occurrences in regions adjacent said location along said selected pattern. 49. The method according to claim 42 wherein in the step of introducing particulate sources of radiation, the particulate sources are introduced by peripheral venous injection to pass through the capillary beds of the body of the subject to be detected in an artery of interest. 50. The method according to claim 42 wherein in the step of detecting radiation, detecting	20
25	gamma rays. 51. The method as in claim 50 wherein in the step of detecting, detecting only pairs of gamma rays received from the body of the subject in substantial coincidence from substantially opposite directions with respect to the selected vessel to produce said signals indicative of said locations.	25
30		30
35		35
40	relative frequency of occurrence of said accumulated numbers of pairs per unit length of the particular vessel. 55. The method as in claim 54 comprising the additional step of analyzing the relative frequency of occurrence of said accumulated numbers of pairs per unit length of said particular vessel to indicate in direct relationship thereto the relative internal cross-sectional areas along	40
45	the length of said particular vessel. 56. Particles for interaction with apparatus as in claim 1 which can be introduced into the blood of a subject, the particles each having dimensions not greater than approximately 8 microns for passing through capillary beds of the body of the subject.	45
50	58. Particles as in claim 57 wherein the sources of radiation produce gamma rays. 59. Particles as in claim 58 wherein the source of radiation produces gamma ray pairs that propagate substantially in opposite directions from the region of a particle. 60. Particles as in claim 59 wherein said source emits positrons at an energy level of less	50
55	62. Particles for interaction with apparatus as in claim 15 which can be introduced into the blood of a subject, the particles each having dimensions not greater than approximately 8 microns for passing through capillary beds of the body of the subject.	55
60	64. Particles as in claim 63 wherein the sources of radiation produce gamma rays. 65. Particles as in claim 64 wherein the source of radiation produces gamma ray pairs that propagate substantially in opposite directions from the region of a particle. 66. Particles as in claim 65 wherein said source emits positrons at an energy level of less	60
65	than approximately 1 MeV. 67. Particles as in claim 66 wherein the source of positrons includes Gallium ₆₈ .	65

GB 2 031 142A 11

CLAIMS (19 Feb 1979)
34. Apparatus according to claim 1 substantially as hereinbefore described with reference to the accompanying drawings.

Printed for Her Majesty's Stationery Office by Burgess & Son (Abingdon) Ltd.—1980.
Published at The Patent Office, 25 Southampton Buildings, London, WC2A 1AY, from which copies may be obtained.